Quality time for better care

"Quality time for better care" is the brand promise of Terumo Medical Care Solutions.

TERUMO MEDICAL CARE SOLUTIONS


HOSPITAL CARE

Surshield™ Versatus™


Safety I.V. Catheter

Disinfect the puncture site according to local hospital policy and make sure all items are ready.
Do not touch the catheter prior use.
Always consult your facility approved protocol or CDC guidelines.

1 Preparation

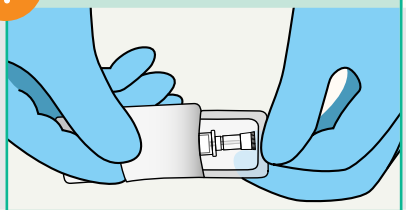


Remove the I.V. catheter from the packaging.

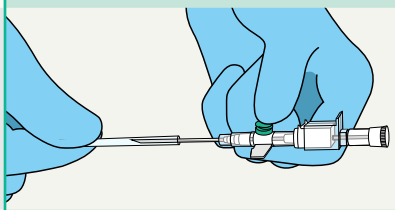


Hold the device from the hub and remove the needle protector with a rotating gesture.


2 Placement

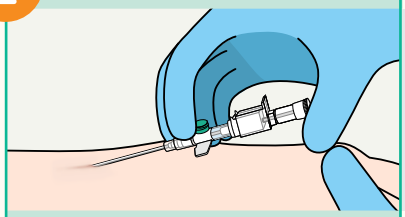

After skin disinfection and tourniquet application, insert the cannula into the vein at a low entrance angle.

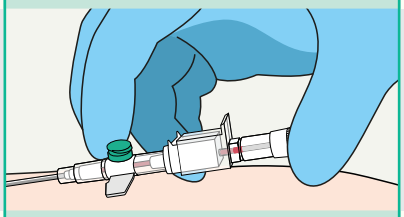


Check blood flow and its level in the flashback.

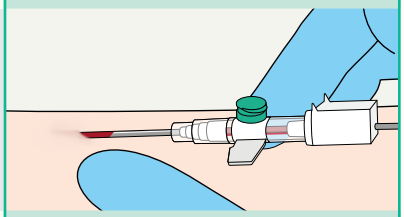


Check also blood presence at the insertion point ('Secondary flashback').

3 Retraction and disposal

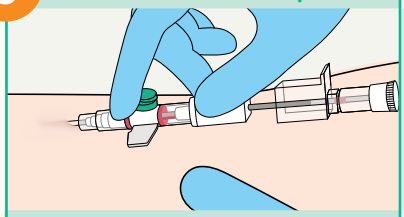

Either fix or hold the cannula with fingers before completely retracting the needle.

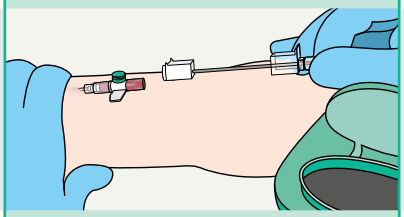

Maintain venous digital pressure, extract completely the needle and throw it away in a sharps container.

Use proper dressing regimes to fix the catheter according to hospital guidelines.

Recommendations for use

Please always consult the product label for a complete overview of warnings, cautions and precautions prior to actual use.

MP258GB-0622FK-I(11.22)E

TERUMO EUROPE N.V. +32 16 38 12 11 www.terumo-europe.com